

Gesamtauswertung Probe 1



Teilnehmer- nummer	Formaldehyd	
	Labor- resultat [mg/m ³]	z - score
5	0,115	0,8
19	0,152	2,1
26	0,013	9,0
34	0,115	0,9
86	0,101	2,0
95	0,141	1,2
107	0,112	1,1
111	0,127	0,1
127	0,137	0,9
130	0,133	0,6
150	0,144	1,5
263	0,123	0,2
268	0,126	0,0
271	0,110	1,3

Die mit  gekennzeichneten Felder sind Ausreißer!

	Form- aldehyd
Gesamtmittelwert c_k [mg / m ³]	0,126
Standardabweichung S_k [mg / m ³]	0,015
rel. Standardabweichung [%]	11,91
Mittelwert QS	0,131

Probe 1

Formaldehyd

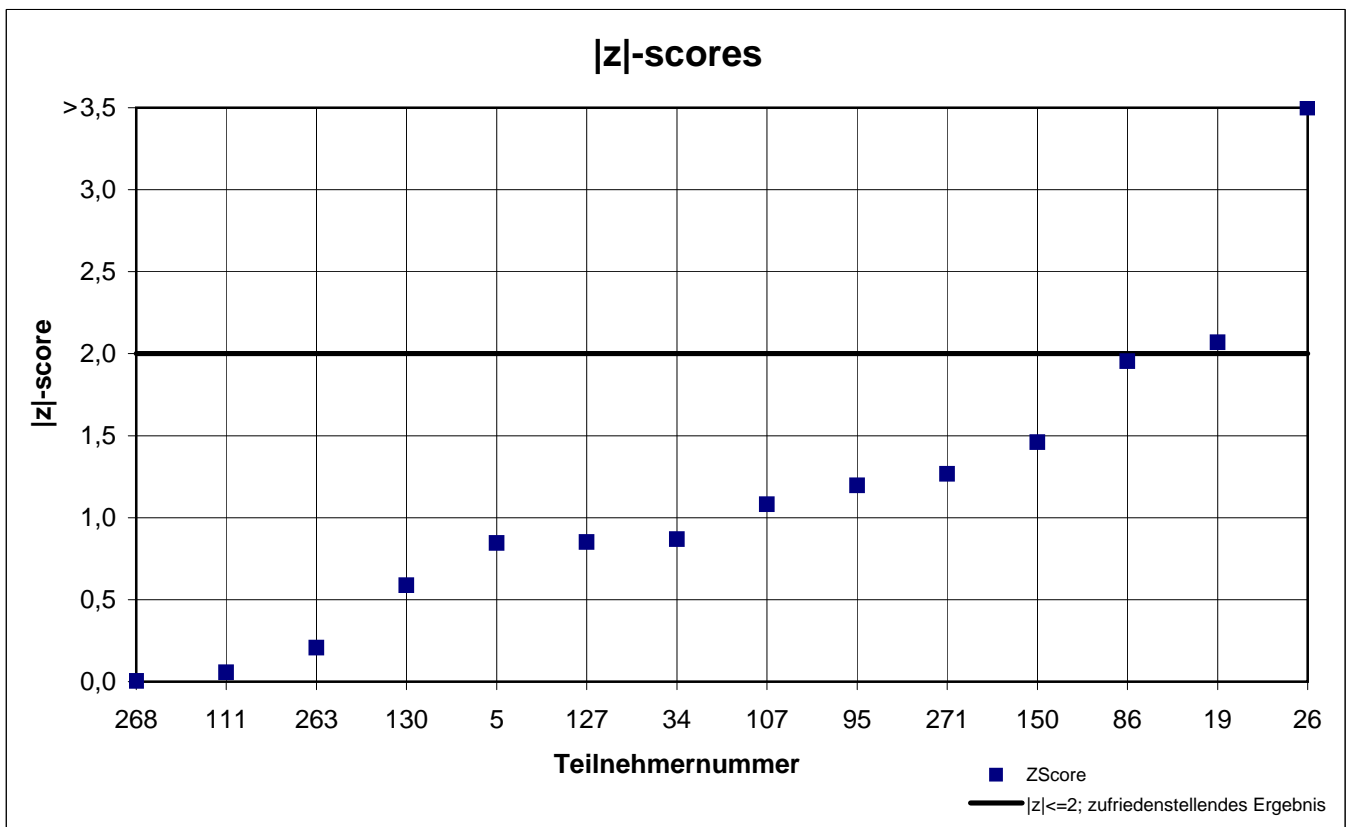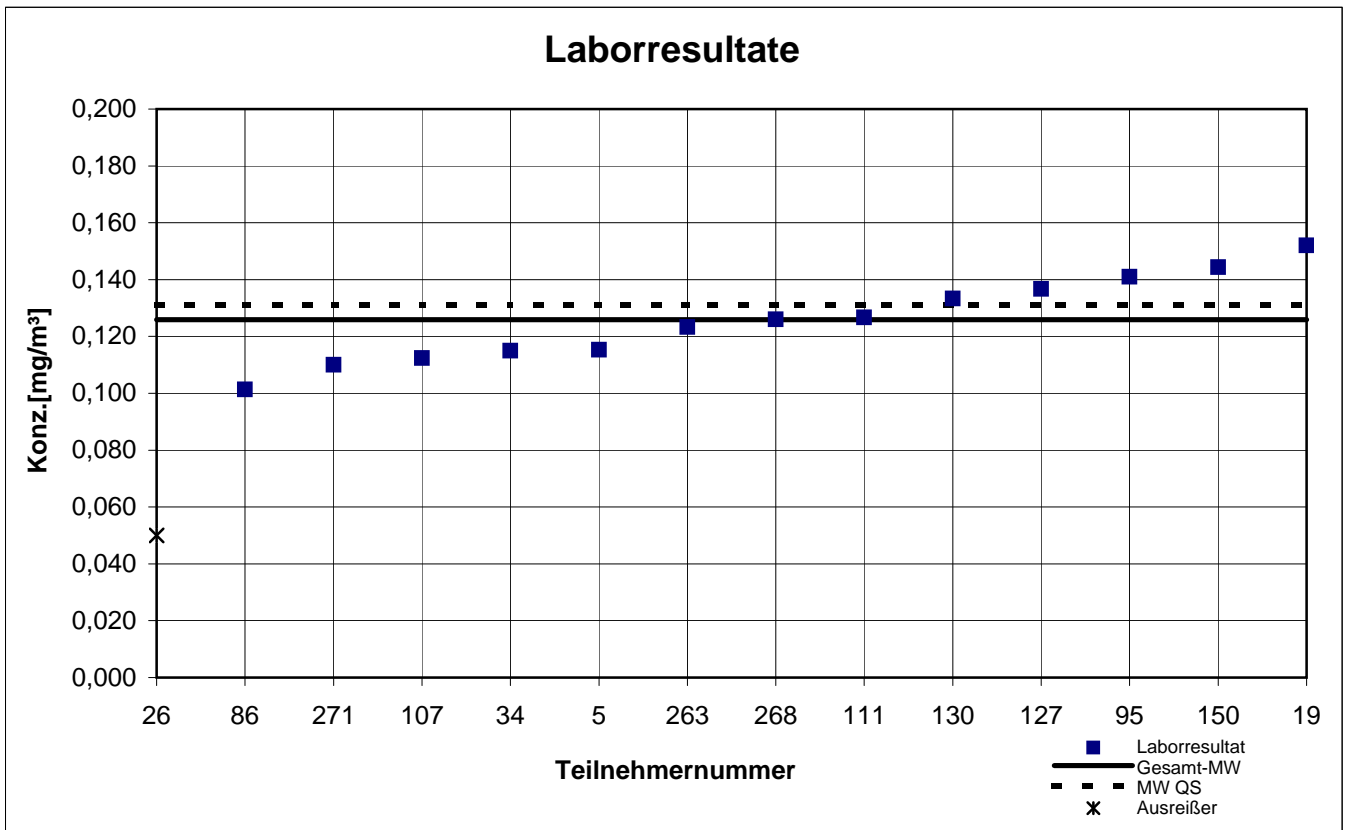

Gesamtauswertung Probe 2



Teilnehmer- nummer	Acetaldehyd		Formaldehyd		Propionaldehyd	
	Labor- resultat [mg/m ³]	z - score	Labor- resultat [mg/m ³]	z - score	Labor- resultat [mg/m ³]	z - score
5	1,621	0,0	0,055	0,7	1,944	0,6
19	1,715	0,6	0,070	1,9	1,990	0,9
26	1,488	0,8	0,060	0,2	1,741	0,5
34	1,868	1,5	0,082	4,0	2,200	2,0
86	1,100	3,2	0,062	0,6	1,000	4,5
95	1,723	0,7	0,063	0,7	2,194	2,0
107	1,560	0,4	0,047	2,1	1,703	0,7
111	1,557	0,4	0,060	0,2	1,750	0,4
127	1,547	0,4	0,066	1,2	1,767	0,3
130	1,627	0,1	0,061	0,3	1,870	0,2
150	1,793	1,1	0,065	1,0	2,000	0,9
263	1,420	1,2	0,055	0,7	1,650	1,0
268	1,493	0,8	0,057	0,3	1,629	1,1
271	0,997	3,8	0,044	2,5	1,350	2,6

Die mit gekennzeichneten Felder sind Ausreißer!

	Acet- aldehyd	Form- aldehyd	Propion- aldehyd
Gesamtmittelwert c_k [mg / m ³]	1,618	0,059	1,830
Standardabweichung S_k [mg / m ³]	0,134	0,007	0,237
rel. Standardabweichung [%]	8,27	12,53	12,97
Mittelwert QS [mg/m ³]	1,358	0,056	1,566



Probe 2

Acetaldehyd

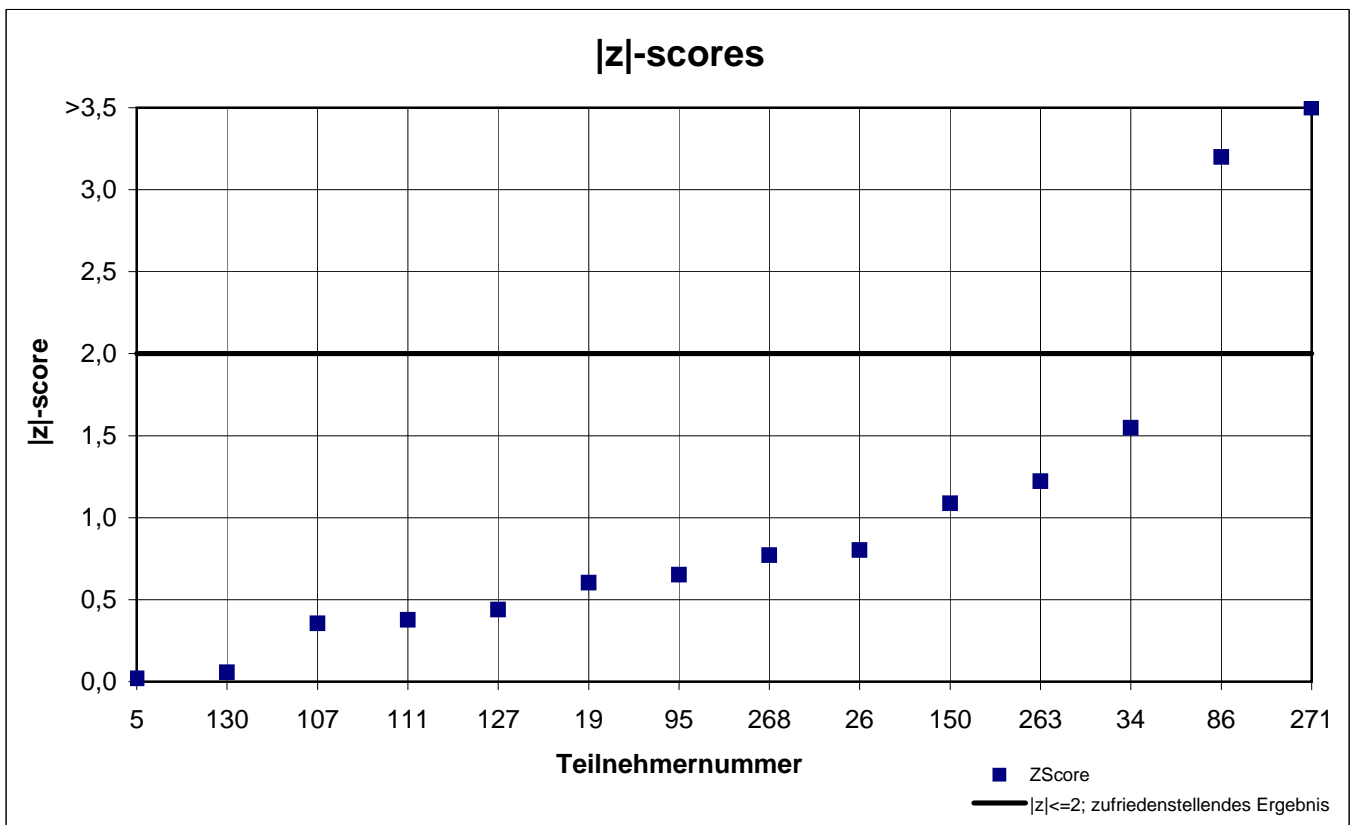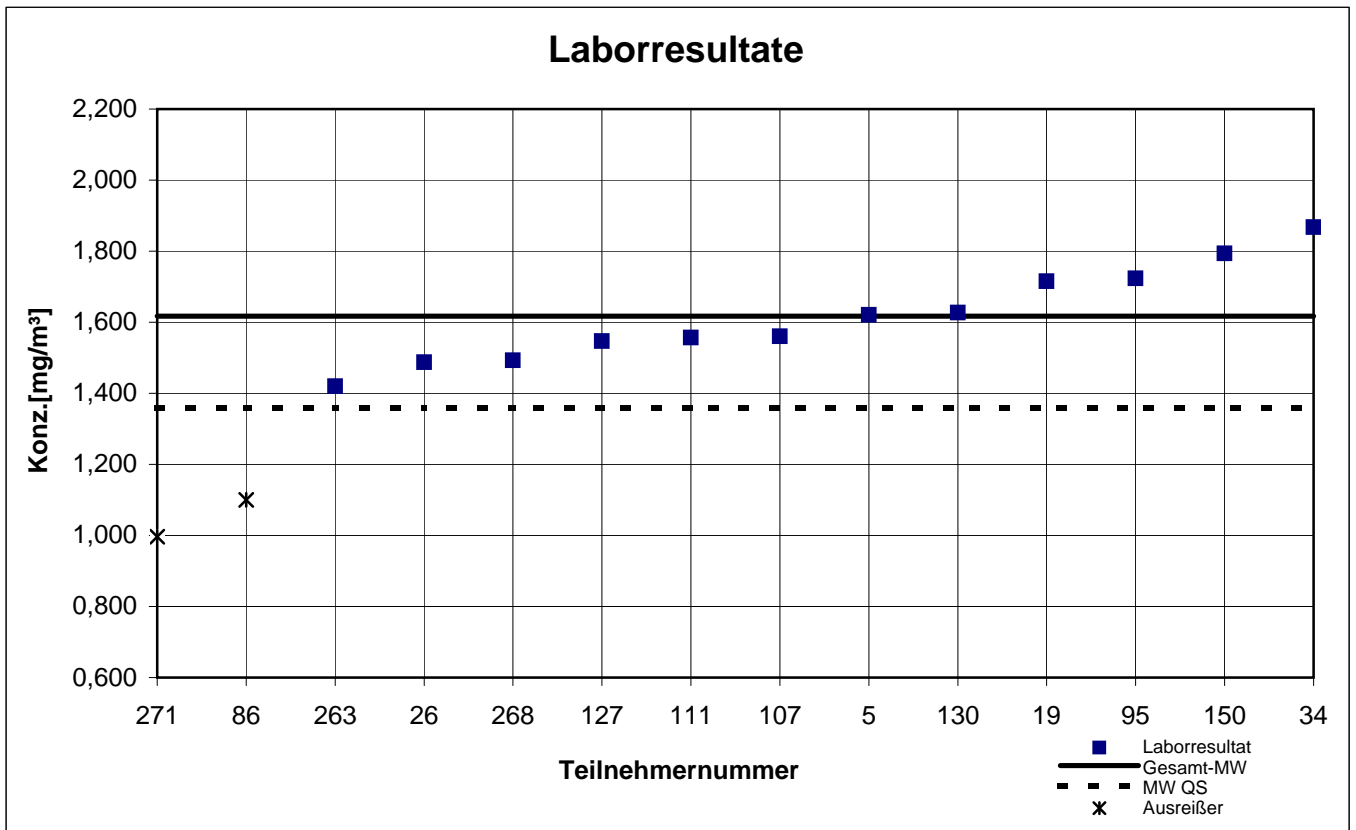



Probe 2

Formaldehyd

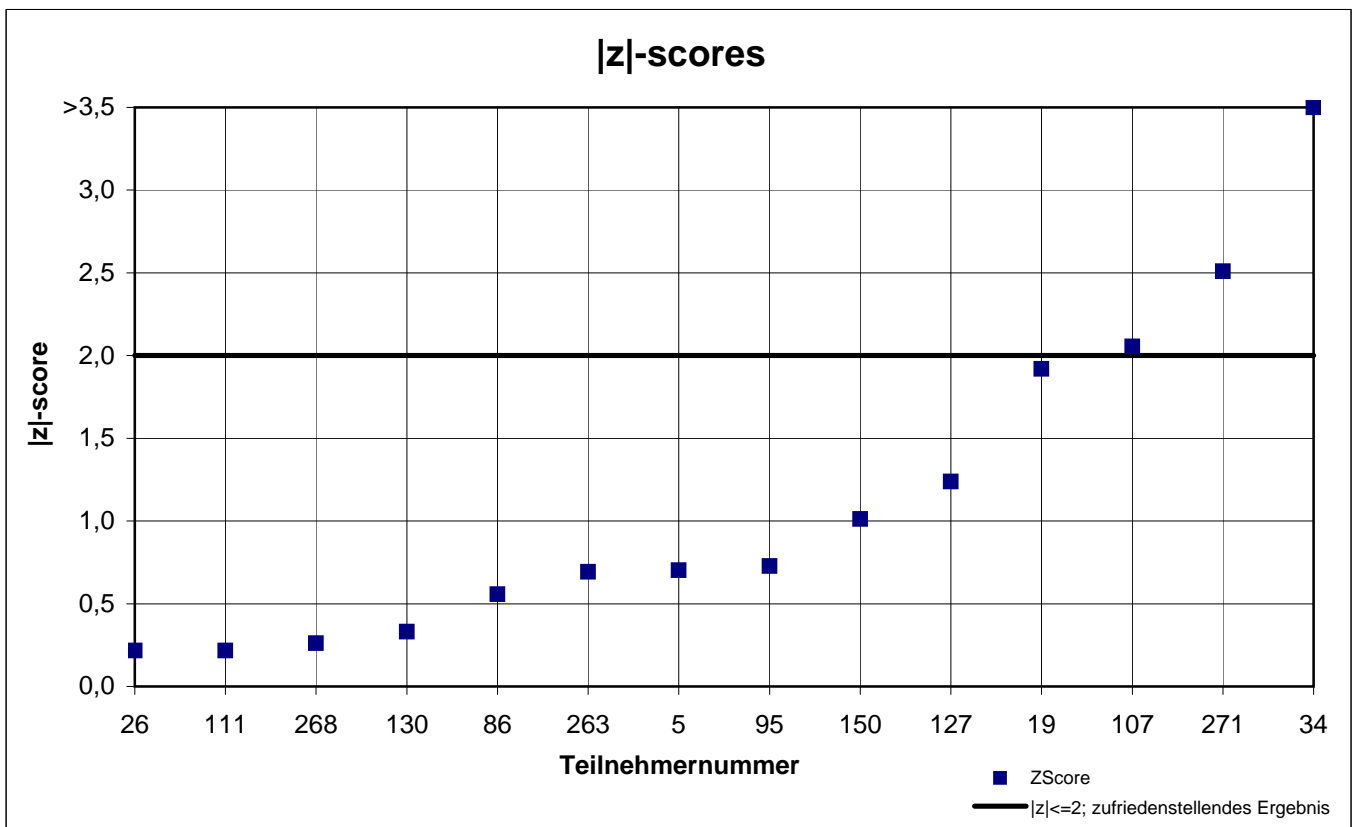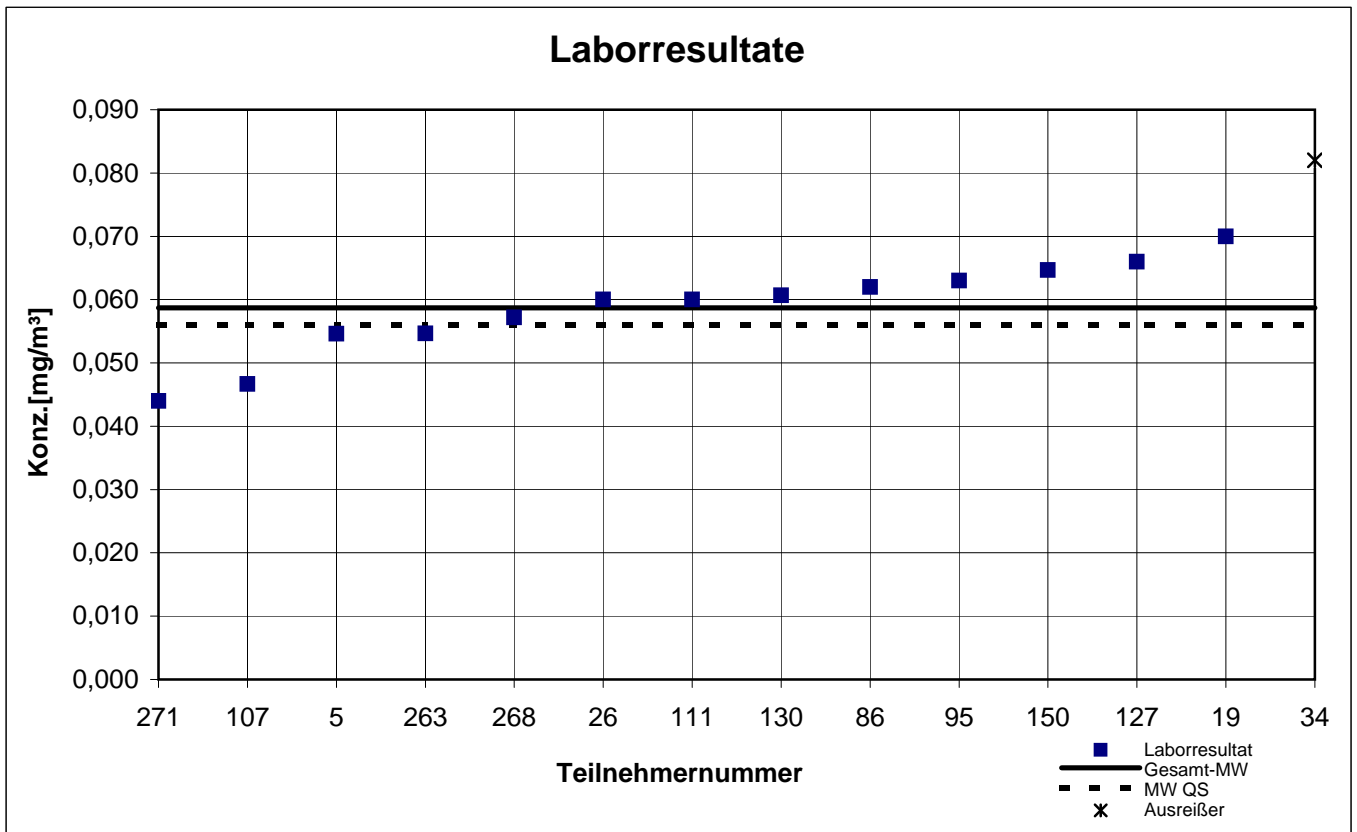

Probe 2

Propionaldehyd

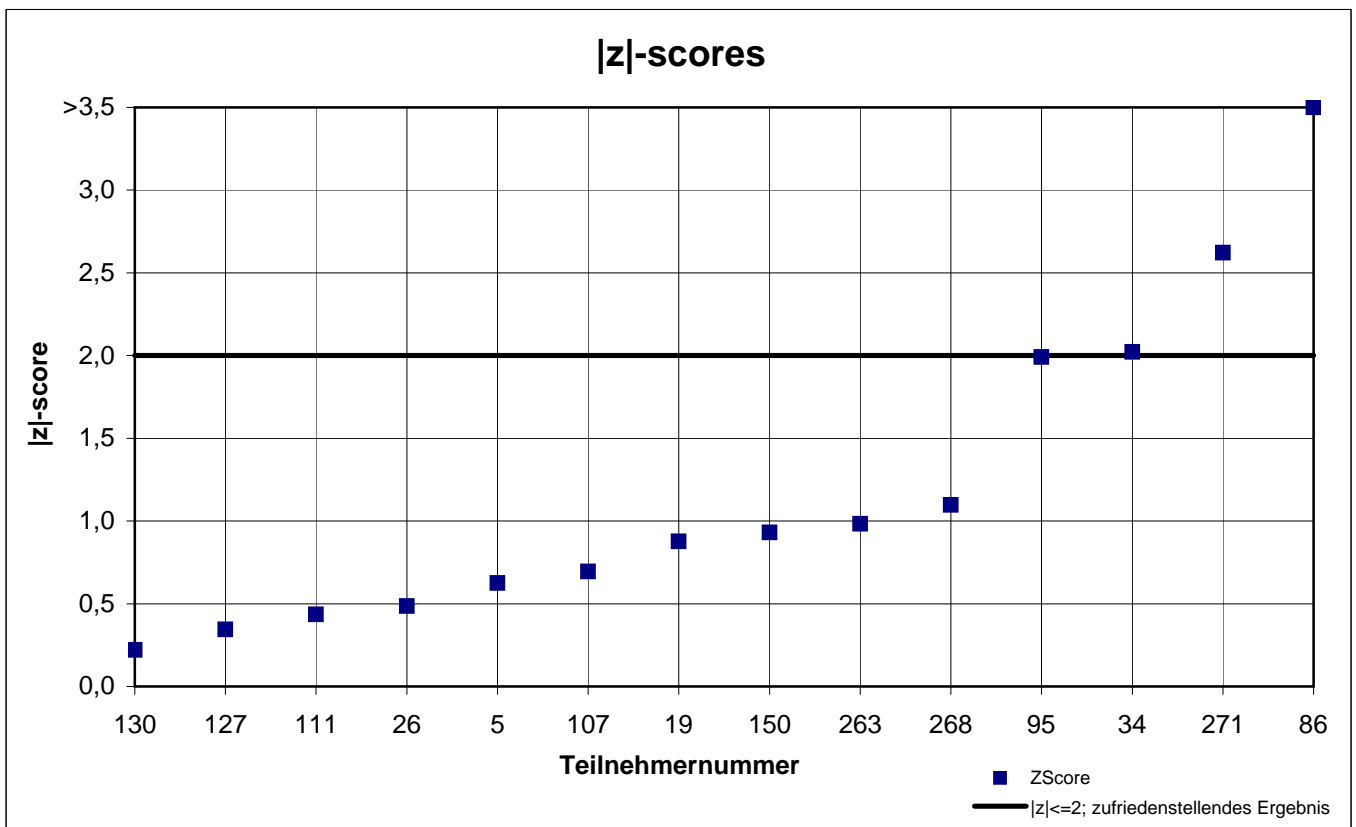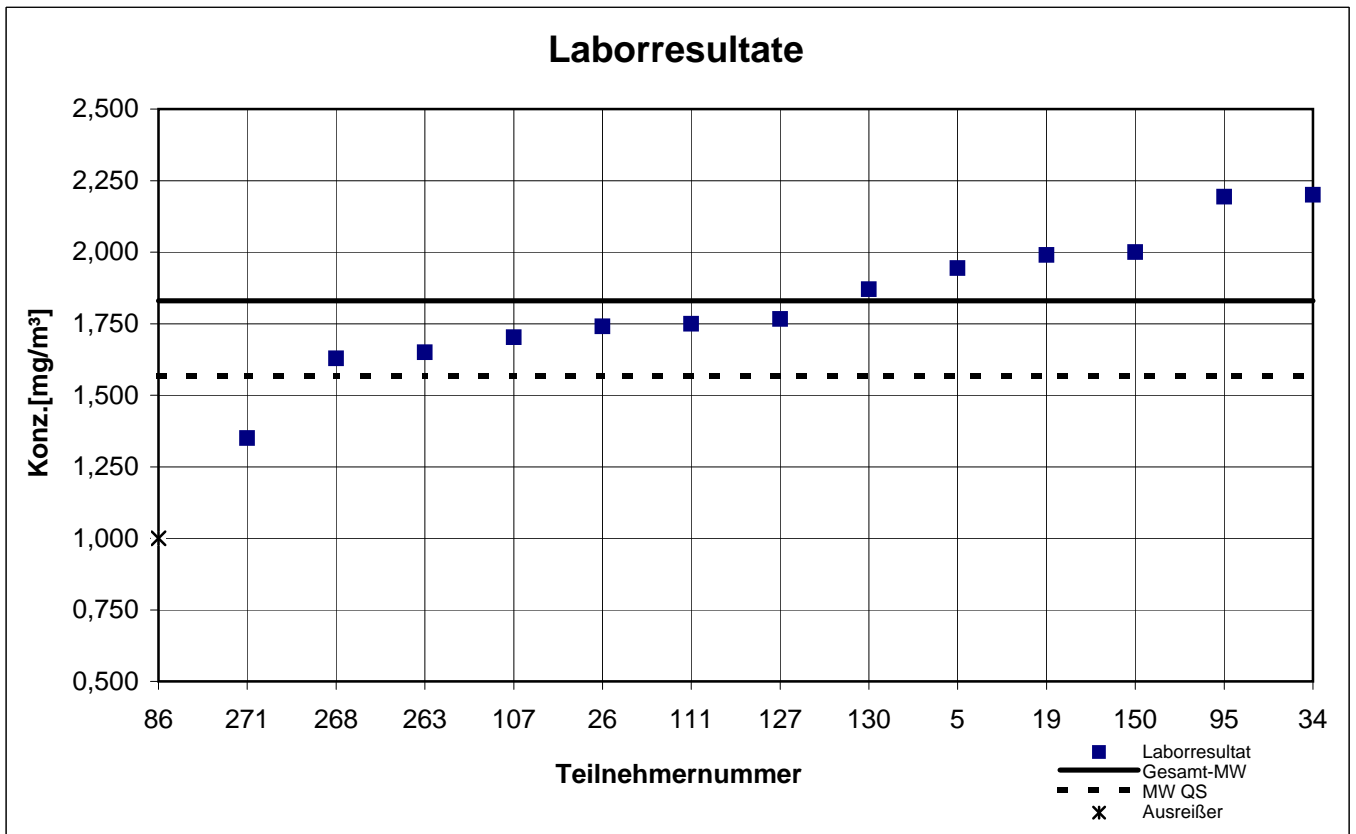

Gesamtauswertung Probe 3



Teilnehmer- nummer	Acetaldehyd		Formaldehyd		Propionaldehyd	
	Labor- resultat [mg/m ³]	z - score	Labor- resultat [mg/m ³]	z - score	Labor- resultat [mg/m ³]	z - score
5	2,548	0,8	0,079	0,8	3,025	1,1
19	2,730	1,6	0,104	2,0	3,175	1,6
26	2,018	1,4	0,086	0,1	2,796	0,2
34	2,291	0,3	0,113	3,1	2,803	0,3
86	1,810	2,3	0,137	5,8	1,670	3,9
95	2,630	1,2	0,089	0,3	3,349	2,3
107	1,366	4,2	0,070	1,9	2,030	2,6
111	2,437	0,4	0,090	0,4	2,730	0,0
127	2,373	0,1	0,088	0,1	2,767	0,1
130	2,473	0,5	0,085	0,2	2,870	0,5
150	2,717	1,5	0,097	1,2	3,087	1,3
263	1,883	2,0	0,078	0,9	2,353	1,4
268	2,338	0,1	0,082	0,5	2,559	0,6
271	0,777	6,7	0,063	2,7	1,990	2,7

Die mit  gekennzeichneten Felder sind Ausreißer!

	Acet- aldehyd	Form- aldehyd	Propion- aldehyd
Gesamtmittelwert c_k [mg / m ³]	2,354	0,087	2,733
Standardabweichung S_k [mg / m ³]	0,308	0,013	0,412
rel. Standardabweichung [%]	13,08	15,19	15,06
Mittelwert QS [mg/m ³]	1,888	0,079	2,386



Probe 3

Acetaldehyd

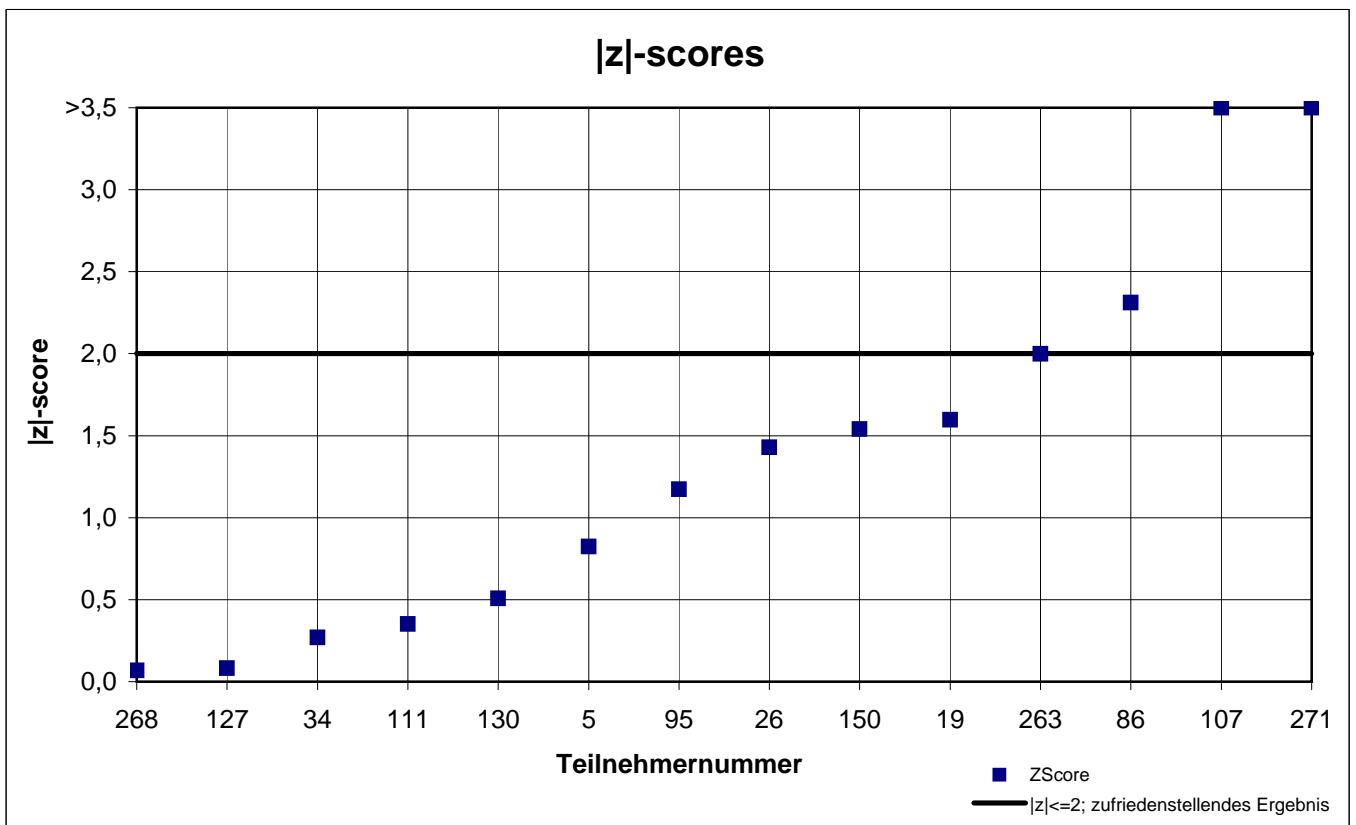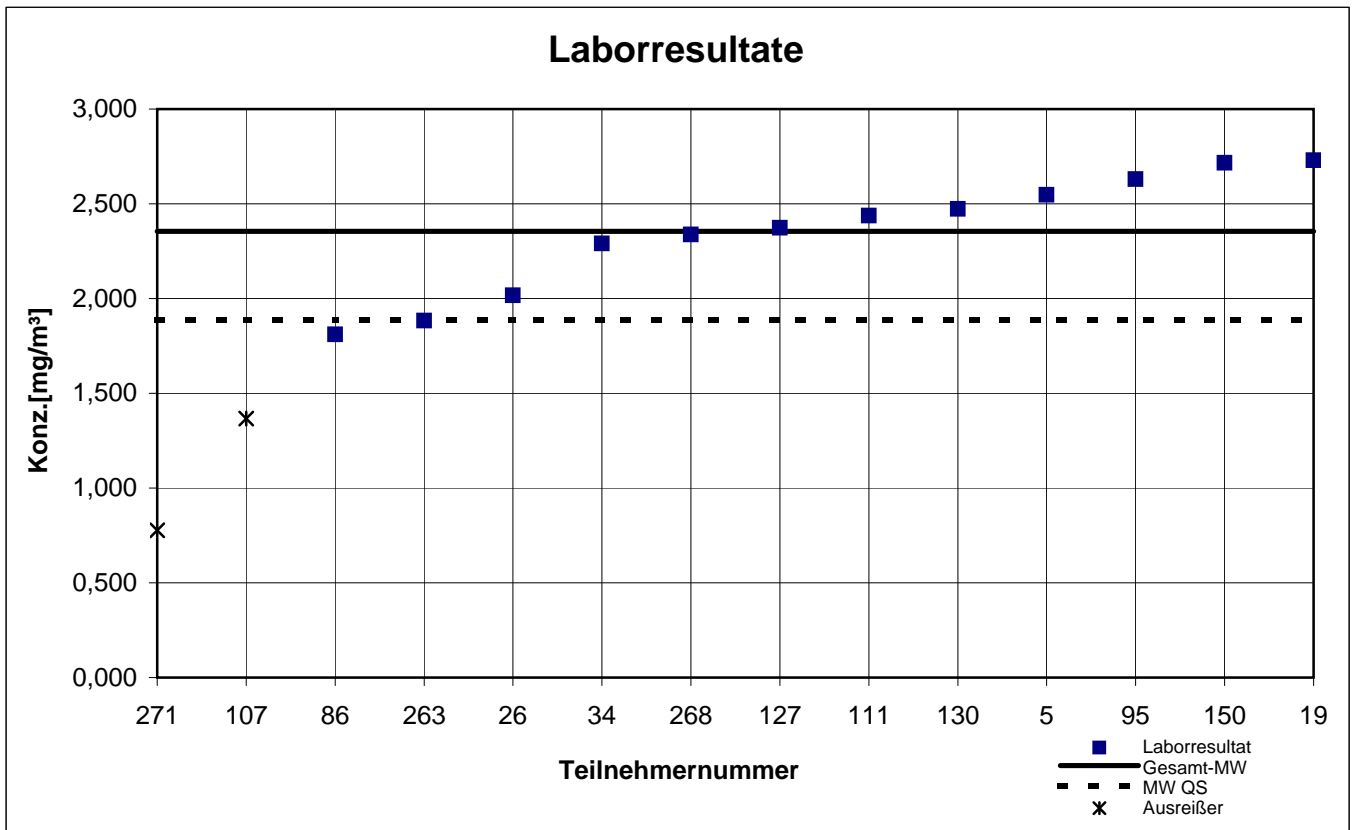

Probe 3

Formaldehyd

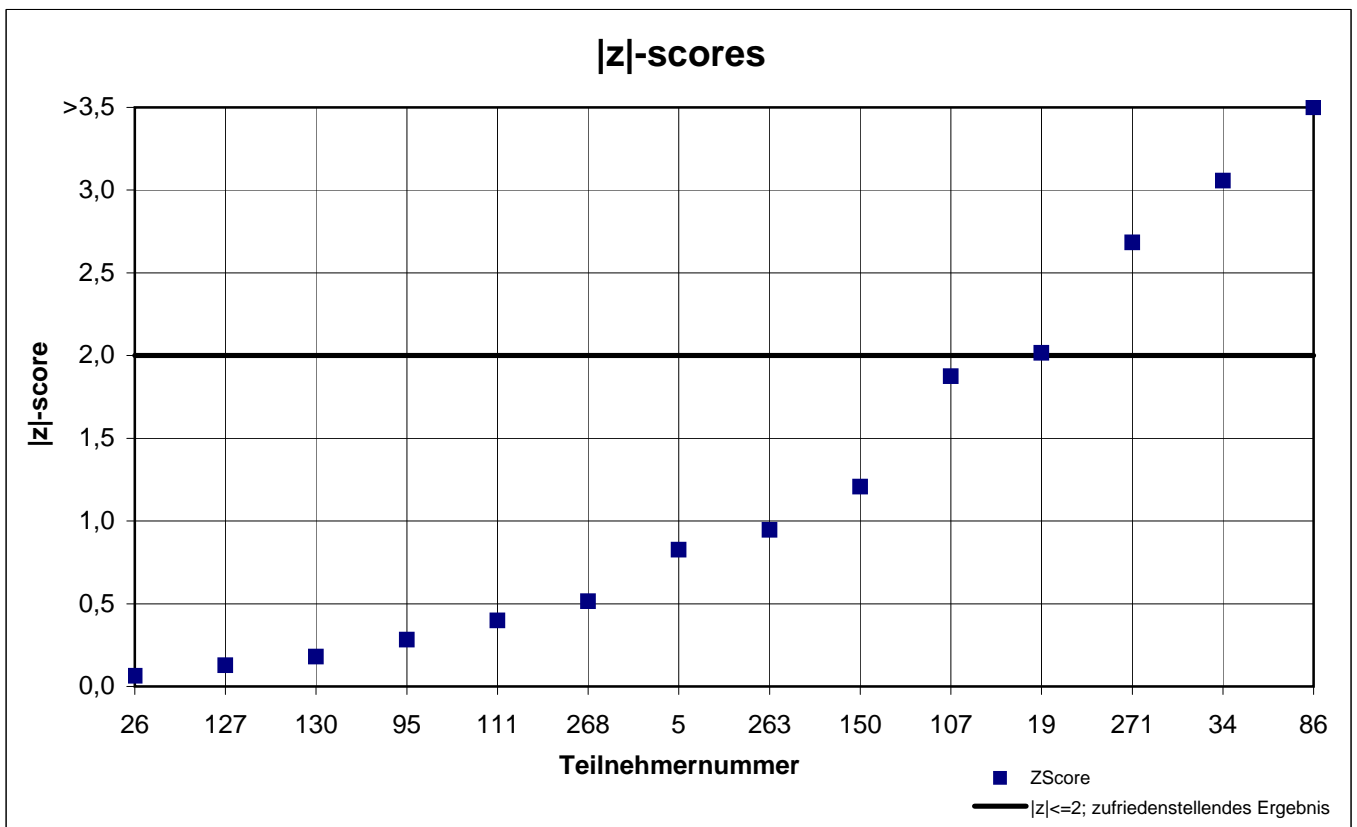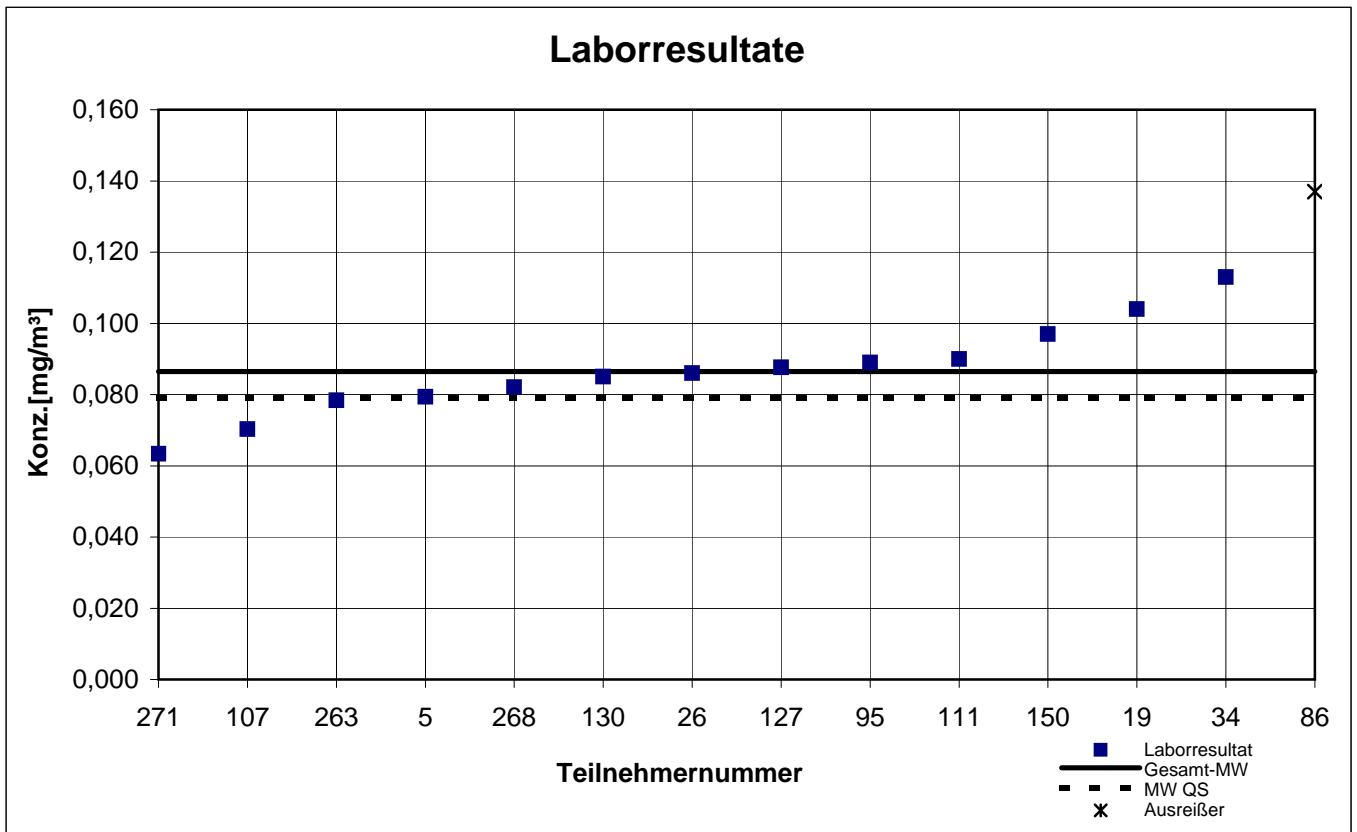

Probe 3

Propionaldehyd

